

Figure 1. Transmittance Detecting System

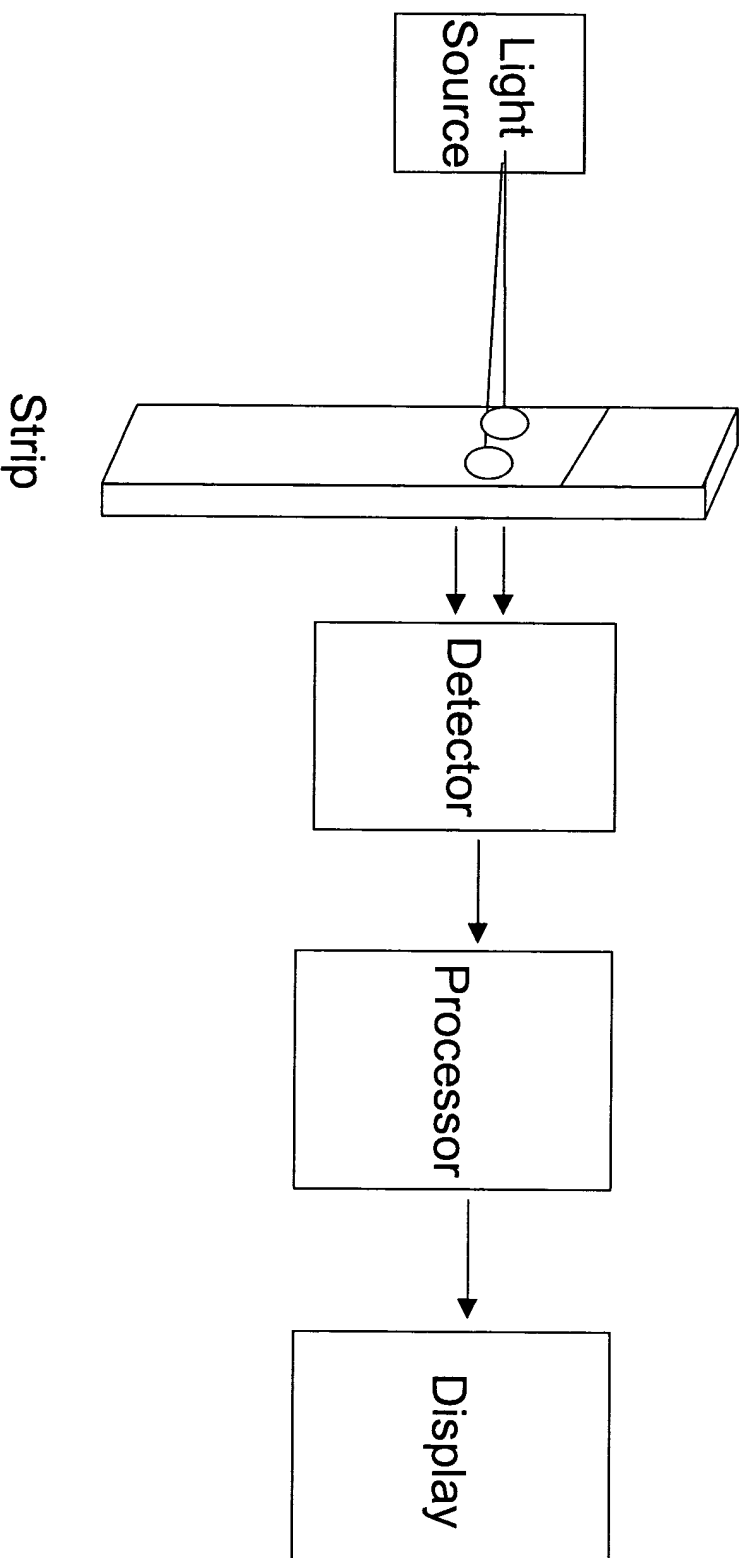


Figure 2. Parallel Cell Arrangement in Chromatographic Strip


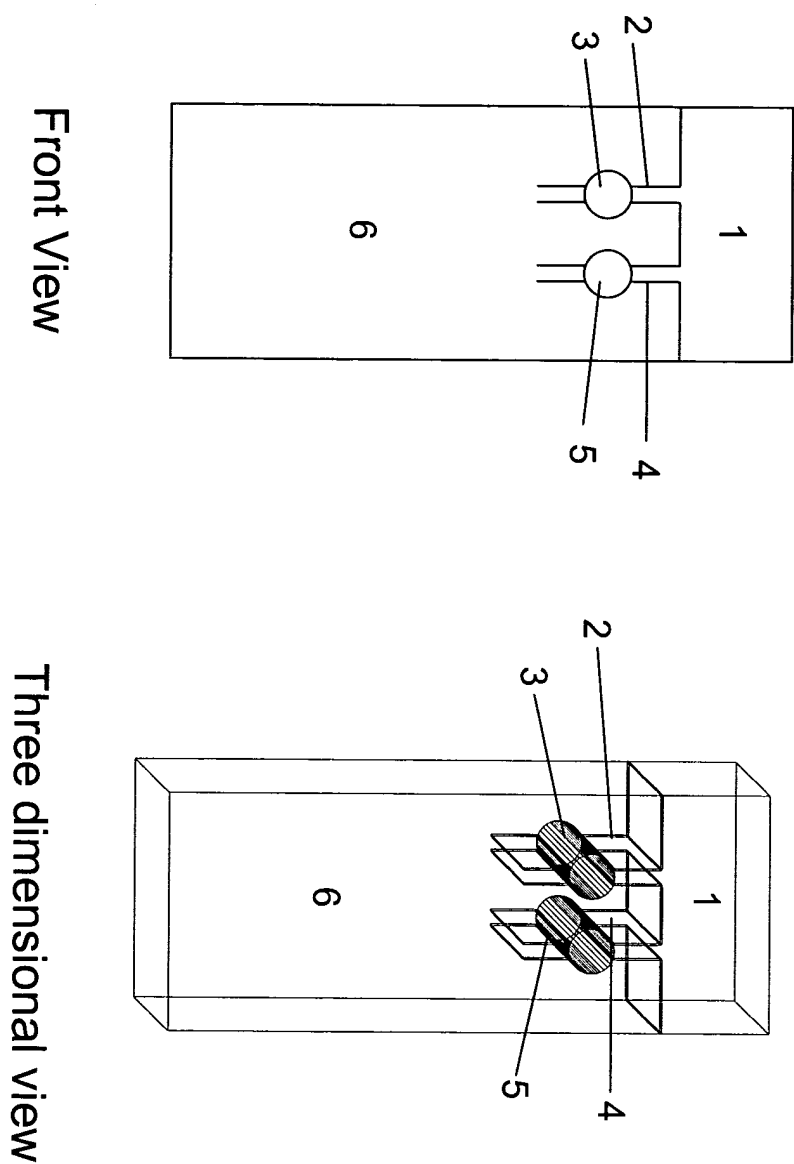


Figure 3. Test Strip Used in Experiment

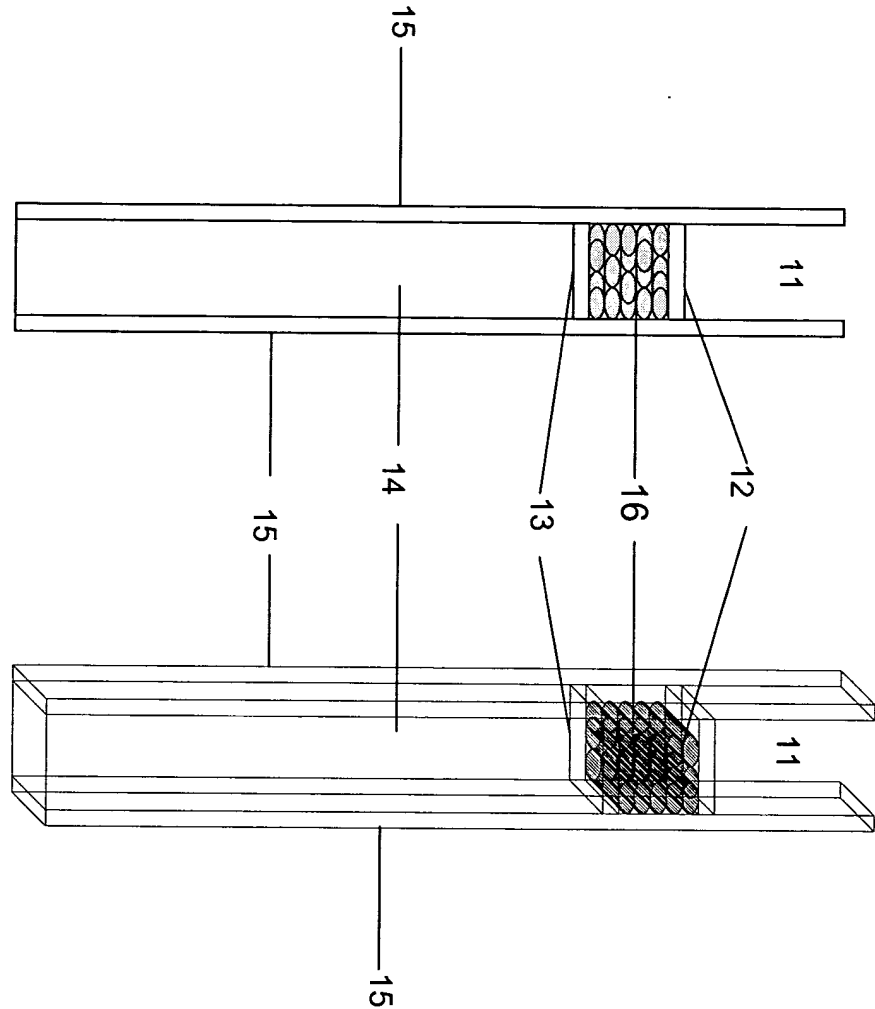

Front view

Three dimensional view

Figure 4. Glycated Hb Measurement Using Chromatographic Strip and Transmittance Detection

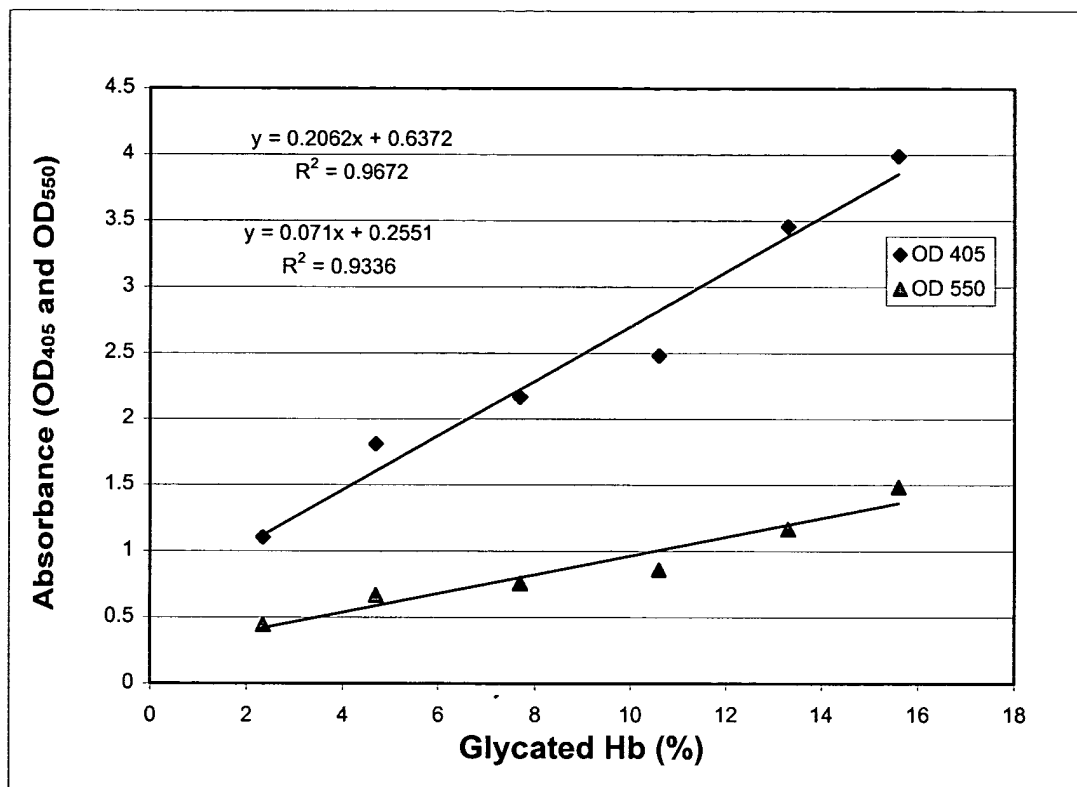


Figure 5. Total Hb Measurement Using Chromatographic Strip and Transmittance Detection

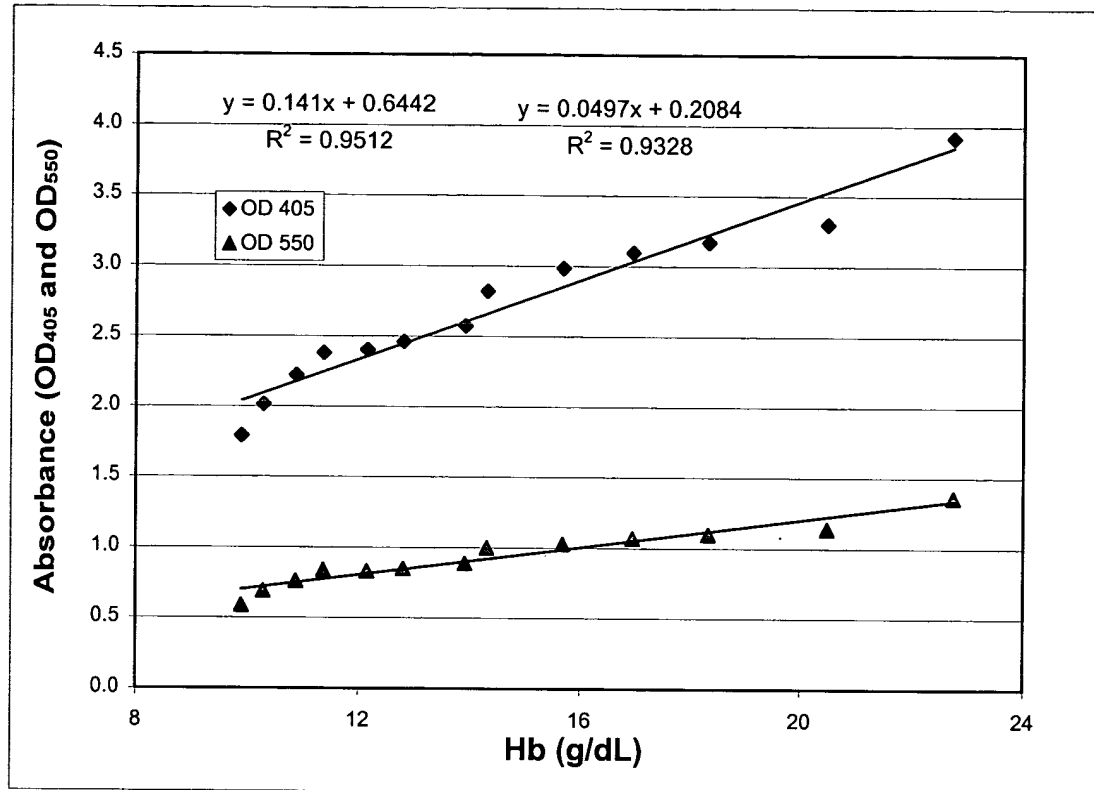


Figure 6. GHb Quantitation by Their Peroxidase Activity

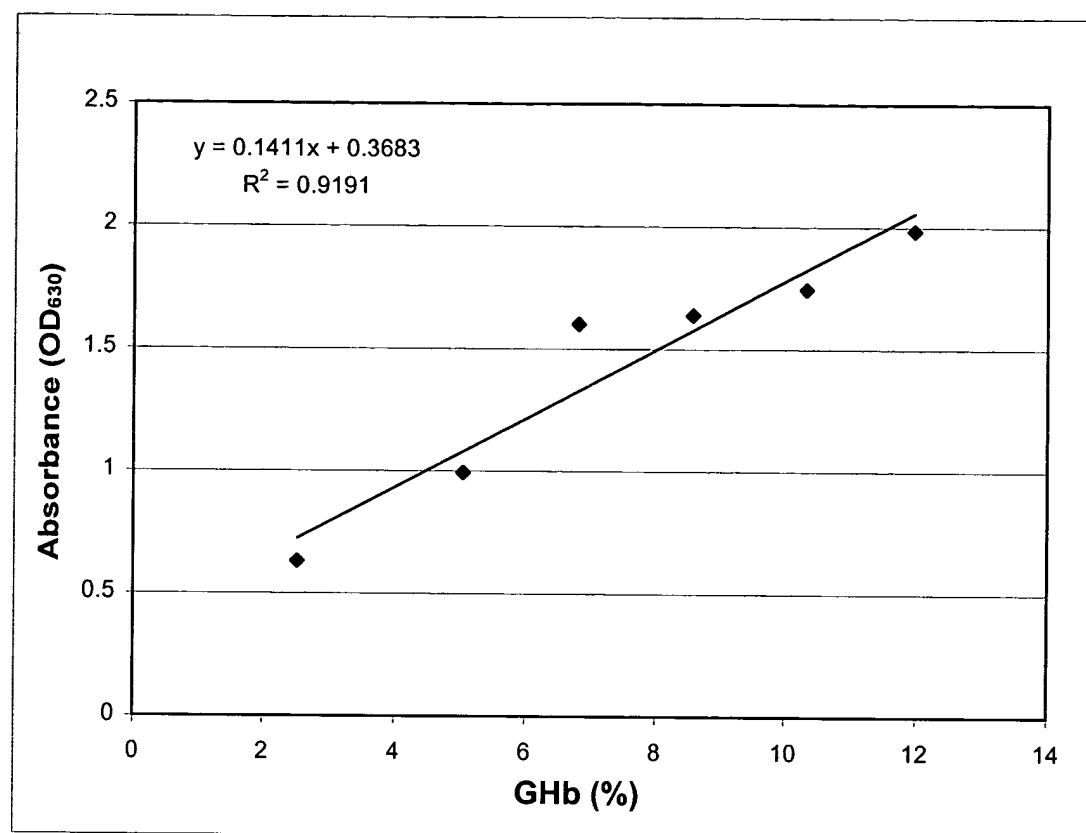


Figure 7. Quantitation of Peroxidase Activity of IgG-HRP Conjugates  
Using Chromatographic Strip and Transmittance Detection

